NMR SPECTROMETRY

Contributor's name and address:	Verification Laboratory DSO National Laboratories 11 Stockport Road Singapore 117605
Secretariat identification code	25-3-0033r (p1/2)
Signature	
Chemical information:	
Chemical name	Bis(2-chloroethyl)sulfone
Schedule number	
CAS registry number	471-03-4
Chemical structure with numbering of atoms	
Molecular formula	$C_4H_8Cl_2O_2S$
Sample information:	
Sample purity	95 %
Sample concentration	16 mg/mL
Solvent	$CDCl_3$
pH	-
Source	In-house synthesis YL21791
Reference chemical shift (internal)	TMS, 0 ppm
Instrument information:	
Manufacturer	Varian, Inc.
Model	Inova 500 MHz
Spectrometer frequency	500 MHz
Software version	VNMR version 6.1C
Experimental information:	
Nucleus measured	^1H
Sample temperature	25 °C
Spectral width (Hz)	5252.1
Data points in Fourier transformed spectrum	32768
Repetition time	12 s
Pulse angle (μs and degrees)	3.462 μs, 45°
Date of experiment	16 Jun 2005
Data points in FID	31480
Number of scans	64
Baseline correction	Yes
Spectral information:	
Chemical shifts (ppm) assigned except for acidic protons	Ha = 3.55, Hb = 3.94
Coupling constants (Hz)	J(a,b) = 6.73
Impurities marked with asterisks	

Bis(2-chloroethyl)sulfone ($C_4H_8Cl_2O_2S$)

[471-03-4]

^{1}H NMR



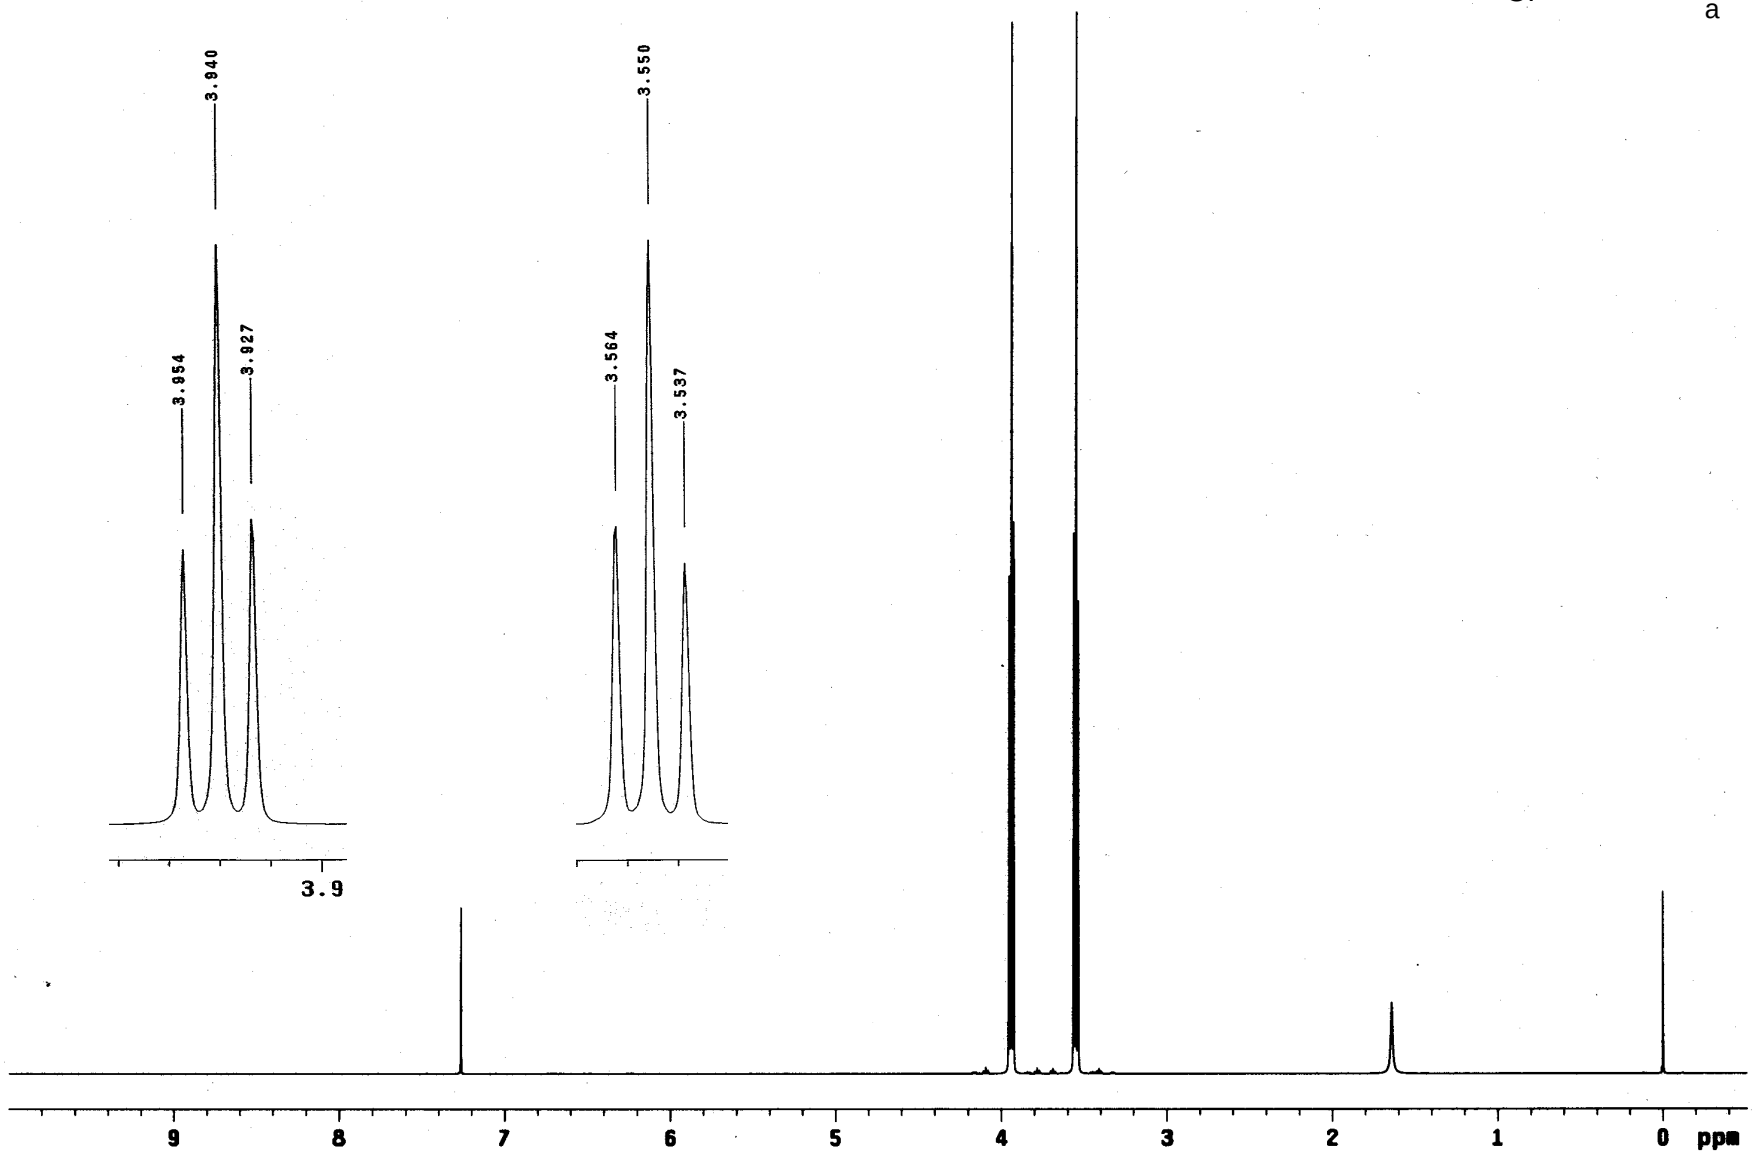

Res.Freq: 499.662 MHz
Solvent: $CDCl_3$
Temperature: 25°C
Concentration: 16 mg/mL

Reference: TMS (internal)
Spectral Width: 5252.1 Hz
Data points [FID]: 31480
Data points [Spectrum]: 32768

Pulse width: 3.462 µs, 45°
Number of Scans: 64
Line broadening: no
Rep. time: 12 s

Resolution: 0.3 Hz (TMS)
Baseline correction: Yes
Instrument: Varian INOVA 500

Nuc	δ[ppm]	J[Hz]
a:	3.55	J(a,b) = 6.73
b:	3.94	