



31P

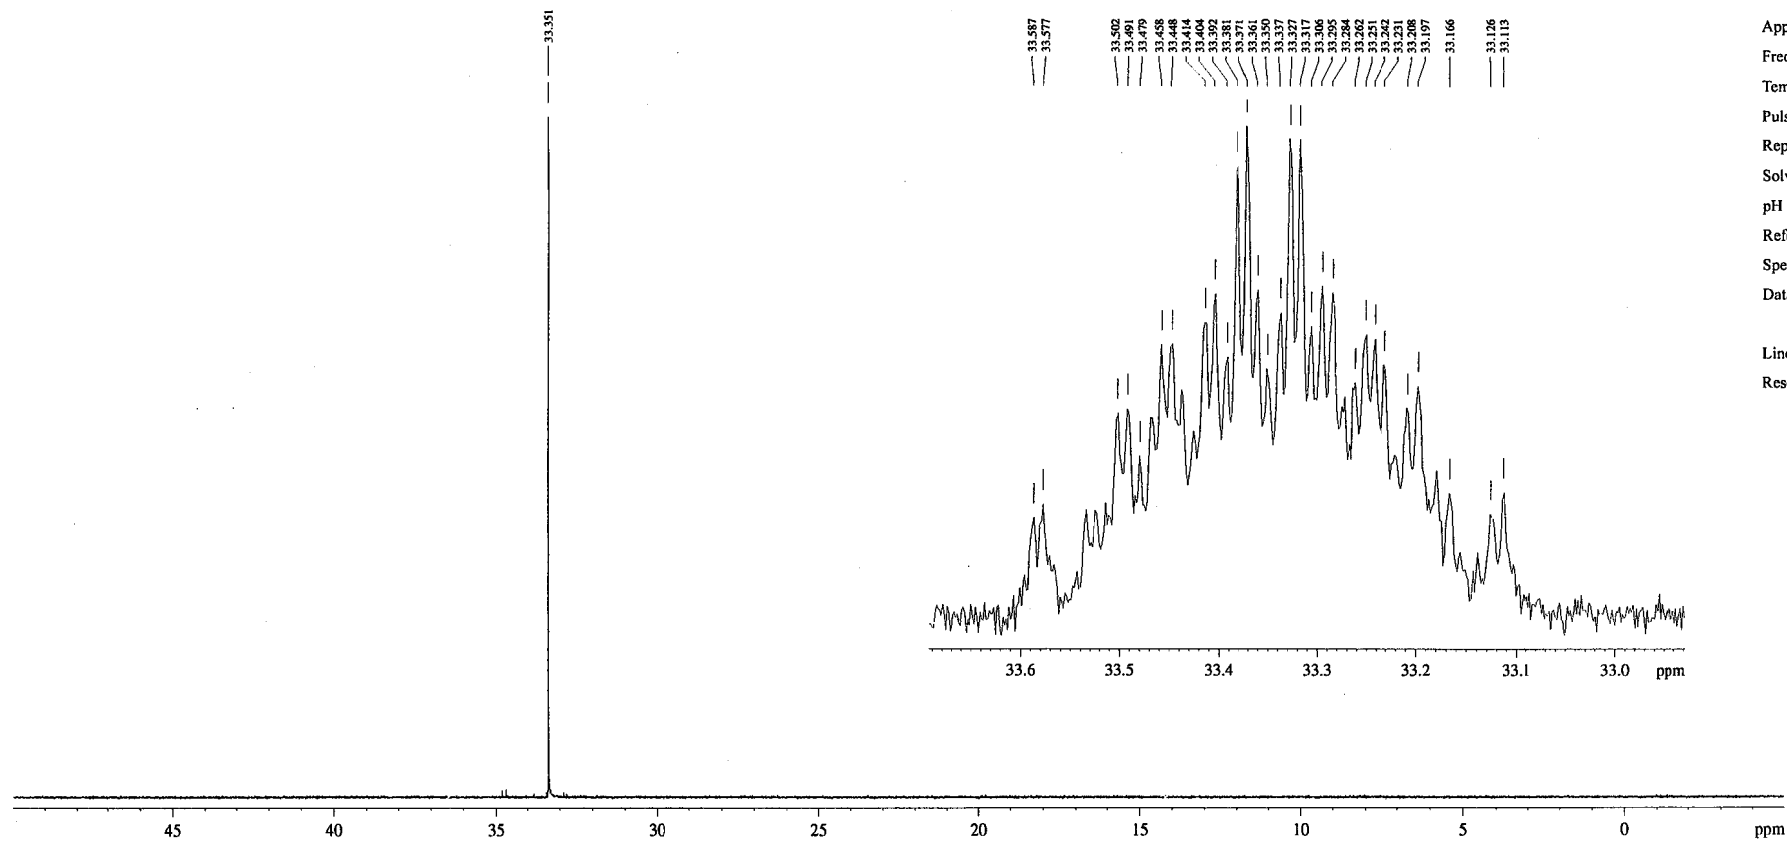

Apparatus : Bruker DPX 360  
Frequency : 145.78 MHz  
Temperature : 25°C  
Pulse Width : 8 μs (90°)  
Repetition Time : 3 s  
Solvent/Lock : D<sub>2</sub>O/D<sub>2</sub>O  
pH : 1  
Reference : H<sub>3</sub>PO<sub>4</sub> external  
Spectral width : 8010 Hz  
Data points : FID = 32K  
SPC = 16K  
Line Broadning : No  
Resolution : peak 33.35 ppm 1.0 Hz

ISOPROPYL PROPYLPHOSPHONATE (pH=1)

MF : C<sub>6</sub>H<sub>15</sub>O<sub>3</sub>P CAS :

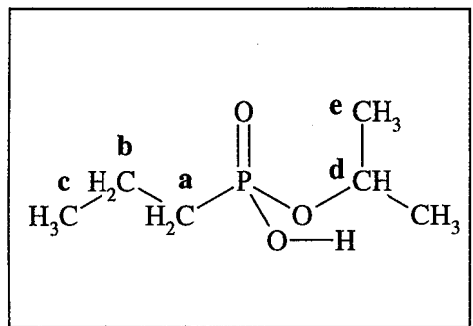

ASSIGNMENT

δ = 33.35 ppm

OPCW Code: 01-3-0286 (p.1/1)