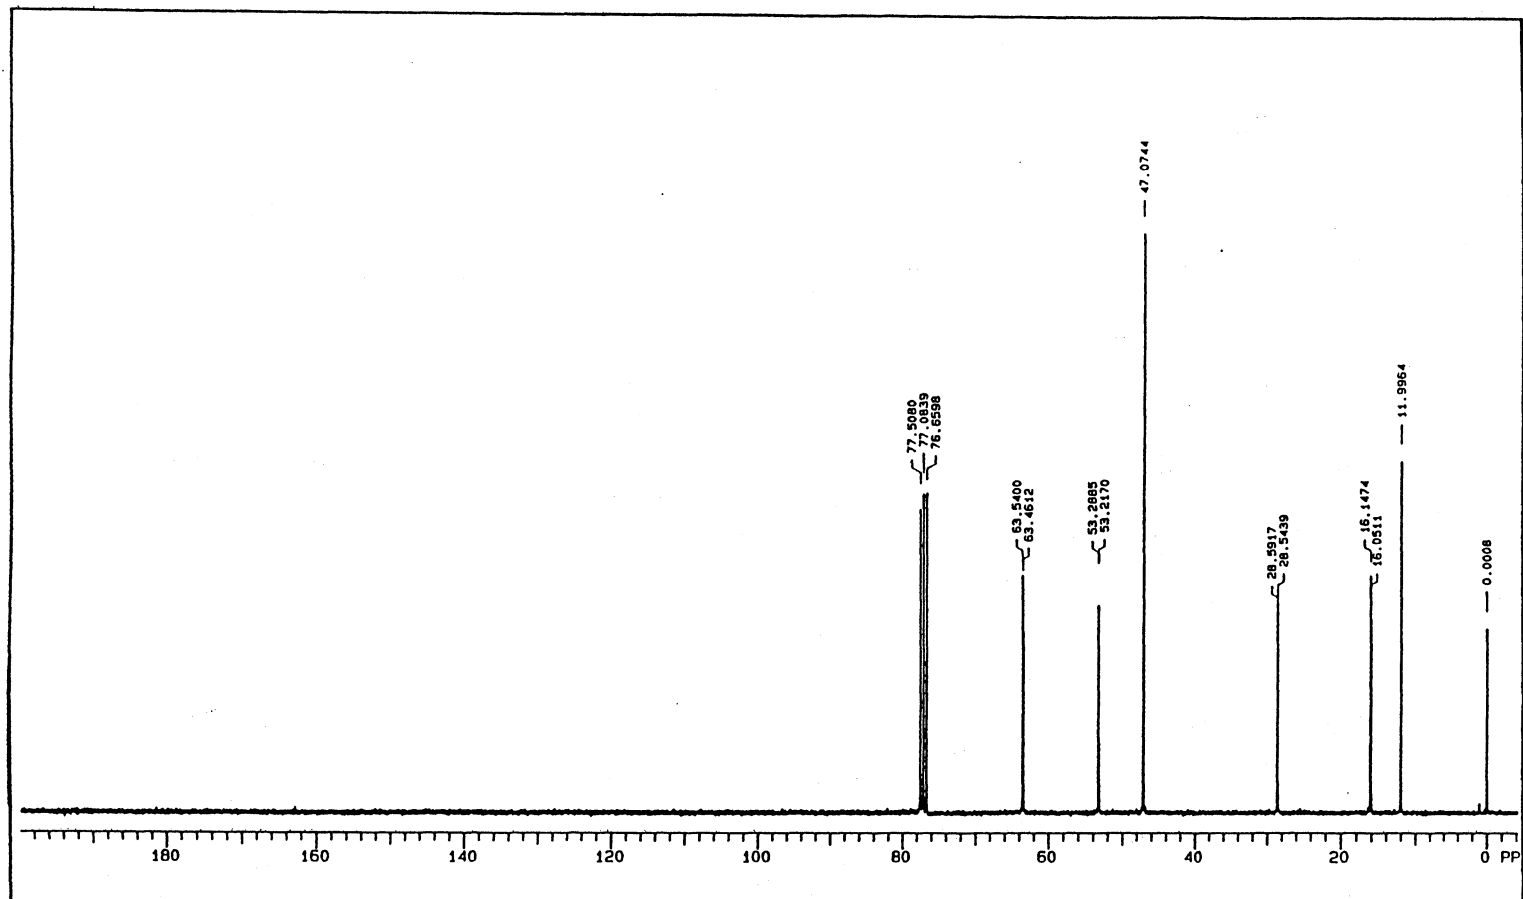
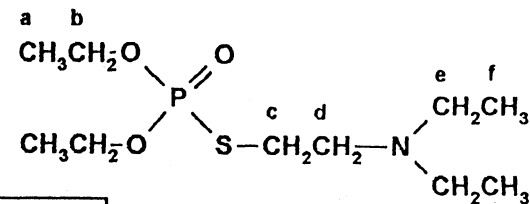


## Amiton

[78-53-5]

 $^{13}\text{C}\{^1\text{H}\}$ -NMRnuc.       $\delta$  [ppm]

a	16.09
b	63.50
c	28.56
d	53.25
e	47.07
f	12.00

J(a,P)	7.1 Hz
J(b,P)	6.0 Hz
J(c,P)	3.6 Hz
J(d,P)	5.4 Hz

Res. freq.    75.429 MHz  
 Solvent:      $\text{CDCl}_3$   
 Temperature: 24°C  
 Concentration: approx. 100mg/ml  
 Reference:    TMS (internal)

Spectral width: 17986 Hz  
 Data points (FID): 64K  
 Data points (spec.): 32K  
 Pulse width: 5.5  $\mu\text{s}$  (38°)  
 Number of scans: 161

Rep.time.: 1.82 s  
 Line broad.: exp., 0.5 Hz  
 Resolution: 1.09 Hz (TMS)  
 Instrument: Varian VXR-300  
 Filename: AM1314/94